


# Microphone Test Report No.:11524



**Ono Sokki**  
**Type: MI-1233**

Serial no: 17326

Sensitivity: 34.6 mV/Pa  
or -29.2 dB re. 1 V/Pa

Date: 2003-08-07


Signature: \_\_\_\_\_

Measurement conditions:  
Polarisation voltage: 0.0 V  
Pressure: 99.86 kPa  
Temperature: 23.1 °C  
Relative humidity: 49.4 %RH  
Results are normalized to the reference conditions.

Free field response  
Diffuse field response  
Pressure (Actuator) response

**Scantek, Inc.**  
7060L Oakland Mills Road, Columbia MD 21046  
Phone 410 290 7726 Service@ScantekInc.com

# Microphone Test Report No.:11524

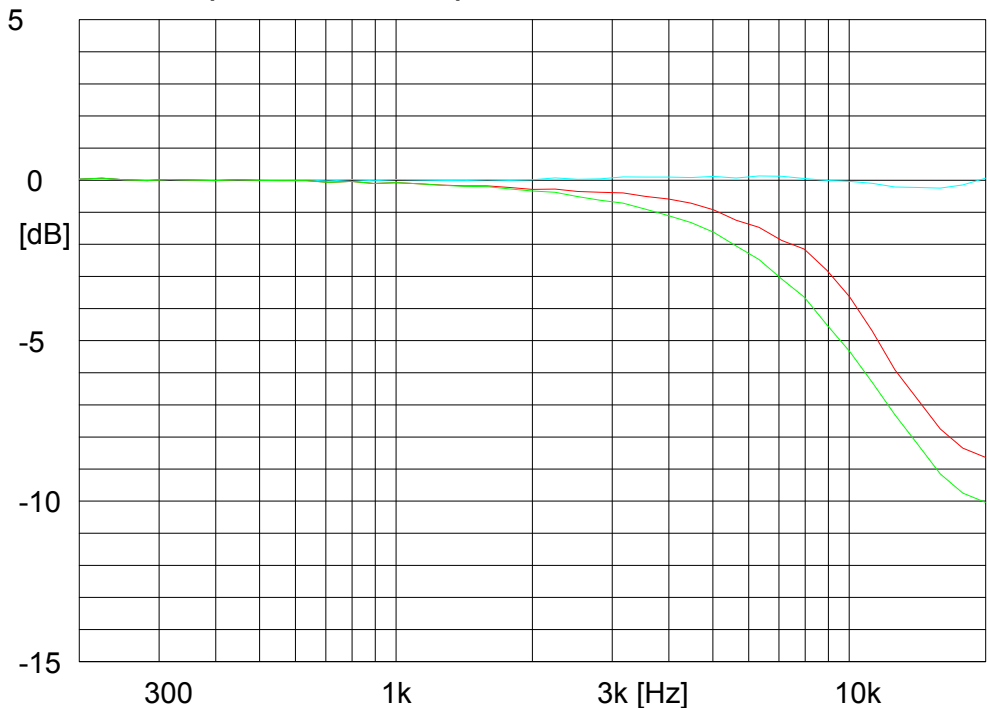

**Ono Sokki**  
**Type: MI-1233**

Serial no: 17326

Sensitivity: 34.6 mV/Pa  
or -29.2 dB re. 1 V/Pa

Date: 2003-08-07

Signature: \_\_\_\_\_

Measurement conditions:  
Polarisation voltage: 0.0 V  
Pressure: 99.86 kPa  
Temperature: 23.1 °C  
Relative humidity: 49.4 %RH  
Results are normalized to the reference conditions.

Free field response  
Diffuse field response  
Pressure (Actuator) response

**Scantek, Inc.**  
7060L Oakland Mills Road, Columbia MD 21046  
Phone 410 290 7726 Service@ScantekInc.com

Comment: